

**BioVendor**

Research  
and Diagnostic Products



## Mouse Insulin High Sensitivity ELISA

Product Data Sheet

Cat. No.: RAI005R

For Research Use Only

## CONTENTS

---

1	INTENDED USE	3
2	PRINCIPLES OF THE TEST	3
3	REAGENTS PROVIDED	3
4	STORAGE INSTRUCTIONS – ELISA KIT	4
5	MATERIALS REQUIRED BUT NOT PROVIDED	4
6	PREPARATION OF REAGENTS	4
7	PREPARATION OF REAGENTS	4
8	TEST PROTOCOL	5
9	CALCULATION OF RESULTS	5
10	TYPICAL STANDARD CURVE	5
11	ASSAY CHARACTERISTICS	6
12	TEST PROTOCOL SUMMARY	8

**»» This kit is manufactured by:  
BioVendor – Laboratorní medicína a.s.**

**»» Use only the current version of Product Data Sheet enclosed with the kit!**

## 1 INTENDED USE

---

This Mouse Insulin High Sensitivity ELISA kit is for the quantitative determination of insulin in mouse serum, plasma and fluid.

## 2 PRINCIPLES OF THE TEST

---

This assay is a two-site ELISA. The micro-plate is pre-coated with a monoclonal antibody against insulin. Standards and samples are added into the wells and co-incubated with a monoclonal antibody conjugated to horseradish peroxidase (HRP) enzyme. After wash step to remove any unbound substances, TMB substrate is added and colour develops in proportion to the amount of insulin bound initially. The assay is stopped and the optical density of the wells determined using a micro-plate reader. Since the increases in absorbance are directly proportional to the amount of captured insulin, the unknown sample concentration can be interpolated from a reference curve included in each assay.

## 3 REAGENTS PROVIDED

---

*Each kit is sufficient for one 96-well plate and contains the following components*

- 1 **Micro-titre Strips (96 wells)**-Coated with a monoclonal antibody against insulin, sealed.
- 1 bottle **Wash buffer (10×)** -30 ml.
- 1 bottle **Assay buffer** - 13 ml, ready for use.
- 1 vial **Detection antibody solution (100×)** -A monoclonal antibody against insulin conjugated to horseradish peroxidase (0.12 ml).
- 1 vial **Insulin standard solutions - 0 ng/ml** (5 ml).
- 5 vials **Insulin standard solutions** - 0.2 ng/ml, 0.5 ng/ml, 1.0 ng/ml, 2.0 ng/ml, 3.5 ng/ml and 7.0 ng/ml (0.15 ml each), ready for use.
- 1 bottle **Substrate solution**- 12 ml, ready for use.
- 1 bottle **Stop solution**-12 ml, ready for use.
- 1 **Plate cover**

## 4 STORAGE INSTRUCTIONS – ELISA KIT

---

The kit should be stored at 2-8°C upon receipt. Remove any unused antibody-coated strips from the micro-plate, return them to the foil pouch and re-seal. Once opened, the strips may be stored at 2-8°C for up to one month.

## 5 MATERIALS REQUIRED BUT NOT PROVIDED

---

- Pipettes and pipette tips.
- 96-well plate or manual strip washer.
- Buffer and reagent reservoirs.
- Paper towels or absorbent paper.
- Plate reader capable of reading absorbency at 450 nm.
- Distilled water or deionized water.
- Horizontal micro-plate shaker capable of 600 rpm.

## 6 PREPARATION OF REAGENTS

---

***Bring all reagents and materials to room temperature before assay.***

### **6.1 Wash Buffer (1x)**

Prepare 1×Wash buffer by mixing the 10×Wash buffer (30 ml) with 270 ml of distilled water or deionized water. If precipitates are observed in the 10× Wash buffer bottle, warm the bottle in a 37°C water bath until the precipitates disappear. The 1×Wash buffer may be stored at 2-8°C for up to one month.

### **6.2 Detection antibody solution**

Prepare 1×Detection antibody solution by dilution of the 100×Detection antibody solution in Assay buffer, mix well. 100 µl of the 1×Detection antibody solution is required per well. Prepare only as much 1×Detection antibody solution as needed. Return the 100×Detection antibody solution to 2-8°C immediately after the necessary volume is removed.

## 7 PREPARATION OF REAGENTS

---

No dilution of the sample is required in this assay, if a sample has an insulin level greater than the highest standard, the sample should be diluted with 0 ng/ml insulin standard solution and the assay should be repeated.

## 8 TEST PROTOCOL

It is recommended that all standards and samples be assayed in duplicate

- a. Add 10  $\mu$ l of standard or sample to its respective well.
- b. Add 100  $\mu$ l of 1x Detection antibody solution per well.
- c. Seal the plate with a plate cover. Incubate at room temperature for 90 minutes, shaking the plate at 600 rpm on a horizontal micro-plate shaker.
- d. Discard the content and tap the plate on a clean paper towel to remove residual solution in each well. Add 300  $\mu$ l of 1x Wash buffer to each well. Incubate at room temperature for 20 seconds. Discard the 1x Wash buffer and tap the plate on a clean paper towel to remove residual wash buffer. Repeat the wash step for a total 4 washes.
- e. Add 100  $\mu$ l of Substrate solution to each well, incubate at room temperature for 15 minutes.  
**Protect from light.**
- f. Add 100  $\mu$ l of Stop solution to each well, gently tap the plate frame for a few seconds to ensure thorough mixing.
- g. Measure absorbance of each well at 450 nm immediately.

## 9 CALCULATION OF RESULTS


- Subtract the absorbance of the blank from that of standards and samples.
- Generate a standard curve by plotting the absorbance obtained (y-axis) against insulin concentrations (x-axis). The best fit line can be generated with any curve-fitting software by regression analysis. Log-log curve fitting or curve of 4-parameter can be used for calculation.
- Determine insulin concentration of samples from standard curve.

## 10 TYPICAL STANDARD CURVE

The following standard curve is provided for demonstration only. A standard curve should be generated for each assay.

Insulin (ng/ml)	Absorbance (450 nm)	Blanked Absorbance
0	0.052	0
0.2	0.063	0.011
0.5	0.098	0.046
1.0	0.197	0.145
2.0	0.558	0.506
3.5	1.23	1.178
7	2.731	2.679

## Insulin standard curve (log-log)

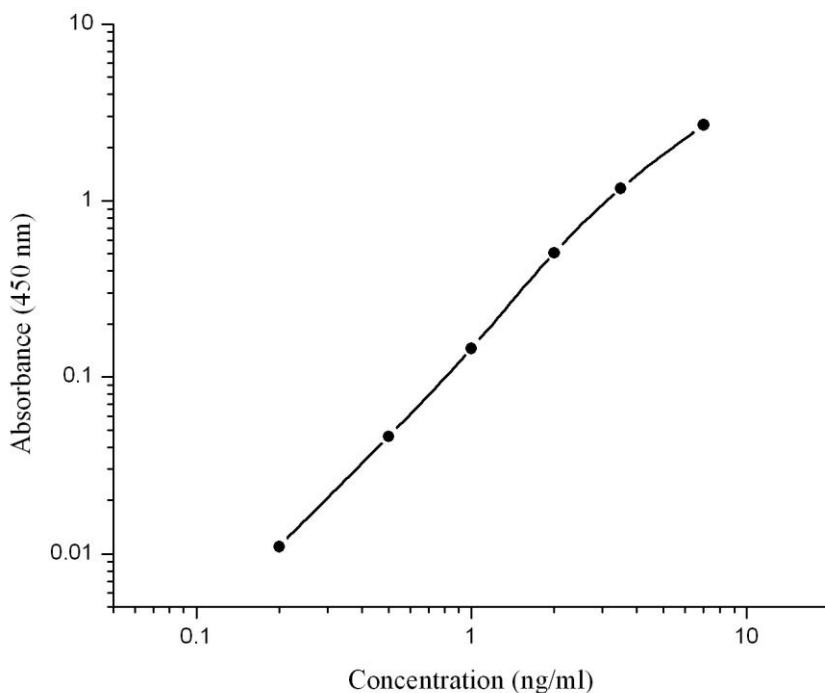

## 11 ASSAY CHARACTERISTICS

### 11.1 Sensitivity

The lowest insulin level that can be measured by this assay is 0.2 ng/ml.

### 11.2 Precision

Intra-assay Precision (Precision within an assay) C.V <10%.

Inter-assay Precision (Precision between assays) C.V <10%.

### 11.3 Recovery

The recovery of the assay was determined by adding various amounts insulin to a sample. The measured concentration of the spiked sample in the assay was compared to the expected concentration. The average recovery was 91%.

### 11.4 Specificity


Percent of cross reactivity

Human insulin 100%

Rat insulin 100%


### 11.5 Validation

Insulin levels were measured at various time points after intra-peritoneal glucose challenge in overnight fasting C57 mice (high-fat fed).

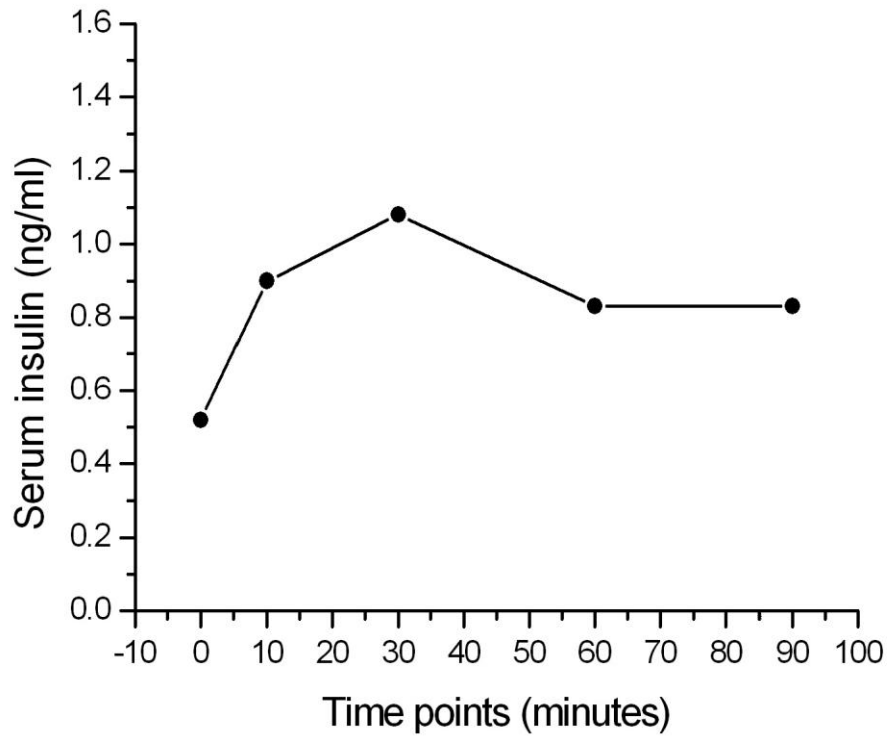


## 12 TEST PROTOCOL SUMMARY

---

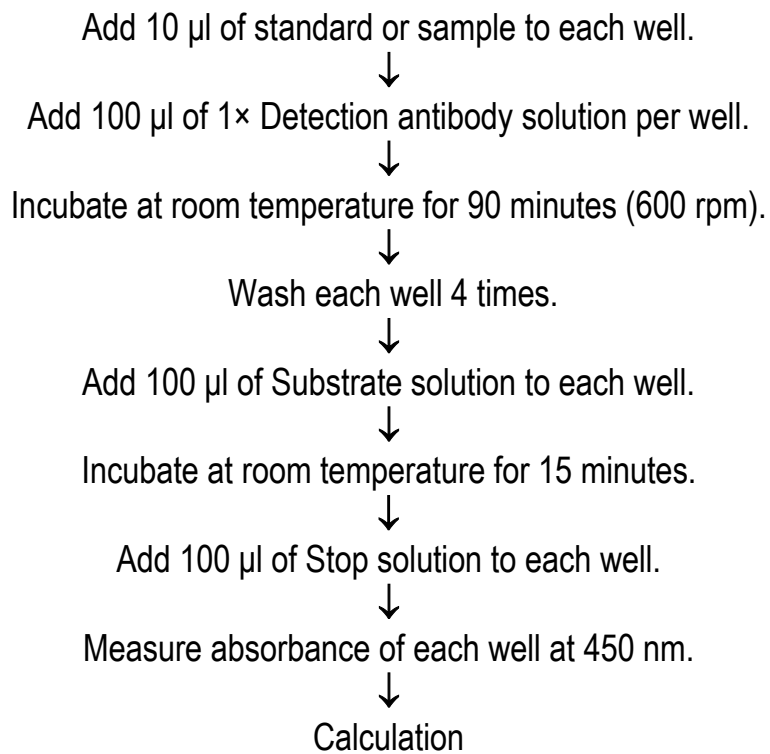



NOTES








# BioVendor

Research  
and Diagnostic Products

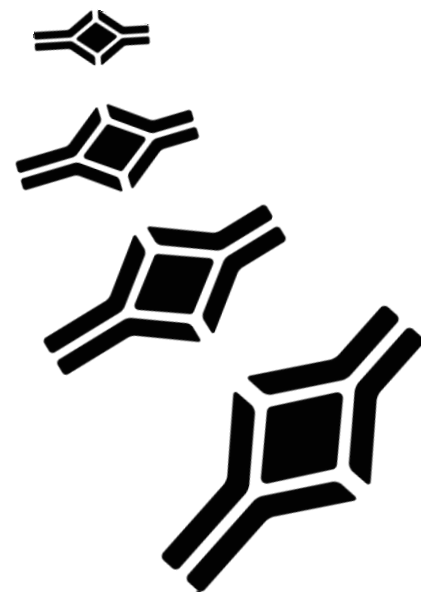

## HEADQUARTERS:

BioVendor - Laboratorní  
medicína a.s.

Karasek 1767/1

621 00 Brno  
CZECH

Phone: +420-549-124-185  
REPUBLIC Fax: +420-549-211-460

E-mail: [info@biovendor.com](mailto:info@biovendor.com)  
[sales@biovendor.com](mailto:sales@biovendor.com)  
Web: [www.biovendor.com](http://www.biovendor.com)

EUROPEAN UNION:  
BioVendor GmbH

Im Neuenheimer Feld 583

D-69120 Heidelberg  
GERMANY

Phone: +49-6221-433-9100  
Fax: +49-6221-433-9111

E-mail: [infoEU@biovendor.com](mailto:infoEU@biovendor.com)

USA, CANADA AND MEXICO:  
BioVendor LLC

128 Bingham Rd.  
Suite 1300

Asheville, NC 28806  
USA

Phone: +1-828-575-9250  
+1-800-404-7807  
Fax: +1-828-575-9251

E-mail: [infoUSA@biovendor.com](mailto:infoUSA@biovendor.com)

CHINA - Hong Kong Office:  
BioVendor Laboratories Ltd

Room 4008  
Hong Kong Plaza, No.188

Connaught Road West  
Hong Kong, CHINA

Phone: +852-2803-0523  
Fax: +852-2803-0525

E-mail: [infoHK@biovendor.com](mailto:infoHK@biovendor.com)

CHINA – Mainland Office:  
BioVendor Laboratories Ltd

Room 2917, 29/F  
R & F Ying Feng Plaza, No.2  
Huaqiang road

Pearl River New Town  
Guang Zhou, CHINA

Phone: +86-20-38065519  
Fax: +86-20-38065529

E-mail: [infoCN@biovendor.com](mailto:infoCN@biovendor.com)